

SEA



RS Calibration
Calibration and Repair Service
Serial No: 18503043
Cert No: 1861041
Cal Date: 24 Apr 2024
Recal Due:

0310
DPN 175 Lammas Road, Corby, Northants, NN17 9RS

****Calibration Certificate****

Do Not Destroy


Calibration Certificate Attached: 1861041
OD ref: 1233975240

5mm Travel Digital Indicator

first

IMPORTANT INFORMATION

Simply detach the label in the top right hand corner of the new front sheet and apply to your instrument as required.

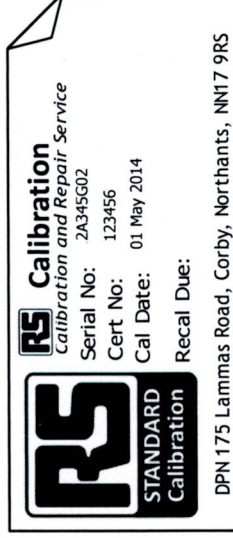

For Re-Calibration of your unit please email:
calibration.uk@rs-components.com
or call us on 01536 405545 to arrange free collection. Please quote serial number when returning.


RS Calibration

CERTIFICATE OF CALIBRATION

Issued by: RS Components Ltd

Date Issued: 24 Apr 2024

Certificate No. 1861041



0310

RS Calibration

Calibration and Repair Service

DPN 175, Lammas Rd,
Weldon Industrial Est
Corby, Northants, NN17 9RS

Tel: 01536 405545
Fax: 01536 401590

Page 1 of 3 Pages

A handwritten signature in black ink, appearing to be 'GC'.

Gary Chadwick

Client

TOTAL LABORATORY SERVICES LTD
BLANDFORD FORUM
DORSET
DT11 8ST

Instrument

5mm Travel Digital Indicator

Serial No.

18503043

Client Reference

N/A

Procedure ID.

D03_1100_# Rev. P4

Date of Calibration

24 Apr 2024

Remarks

This certificate reports recorded values for the instrument 'As Received'.

Uncertainties

The reported expanded uncertainties are based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%. The uncertainty evaluation has been carried out in accordance with UKAS requirements.

For certificate statements of conformity see Appendix SQAR 533
The following calibration results relate only to the items defined above.

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes

This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

CERTIFICATE OF CALIBRATION

UKAS Accredited Calibration Laboratory No. 0310



Calibration and Repair Service

Certificate No.
1861041

Page 2 of 3 Pages

Environment

The ambient temperature and relative humidity throughout the calibration were $(20 \pm 2) ^\circ\text{C}$ and $(40 \pm 20) \%RH$ respectively.

Calibration

The instrument was held in a temperature controlled environment for a period of not less than 4 hours prior to calibration which was performed using a DTI calibration tester and in accordance with RS Calibration procedure MLCP25 and the results compared with the manufacturers specification.

Measured Value (mm)

Repeatability: 0.000

Hysteresis error 0.000

Calibration of indicator:

Tested Size mm	Limit mm	Indicator Reading		Deviation
		mm	mm	
		Up	Down	
0.00	± 0.005	0.000	0.000	0.000
0.20	± 0.005	0.200	0.000	0.000
0.40	± 0.005	0.400	0.000	0.000
0.60	± 0.005	0.600	0.000	0.000
0.80	± 0.005	0.800	0.000	0.000
1.00	± 0.005	1.000	0.000	0.000
2.00	± 0.005	2.000	0.000	0.000
2.50	± 0.005	2.500	0.000	0.000
3.00	± 0.005	3.000	0.000	0.000
3.50	± 0.005	3.500	0.000	0.000
4.00	± 0.005	4.000	0.000	0.000
4.50	± 0.005	4.500	0.000	0.000
5.00	± 0.005	5.000	0.000	0.000
		Down	Down	
5.00	± 0.005	5.000	0.000	0.000
4.50	± 0.005	4.500	0.000	0.000
4.00	± 0.005	4.000	0.000	0.000
3.50	± 0.005	3.500	0.000	0.000
3.00	± 0.005	3.000	0.000	0.000
2.50	± 0.005	2.500	0.000	0.000
2.00	± 0.005	2.000	0.000	0.000
1.00	± 0.005	1.000	0.000	0.000
0.80	± 0.005	0.800	0.000	0.000
0.60	± 0.005	0.600	0.000	0.000
0.40	± 0.005	0.400	0.000	0.000
0.20	± 0.005	0.200	0.000	0.000
0.00	± 0.005	0.000	0.000	0.000

Uncertainty of measurement ± 0.003 mm

CALIBRATED BY:- SEA

CERTIFICATE OF CALIBRATION


UKAS Accredited Calibration Laboratory No. 0310



Calibration and Repair Service

Certificate No.
1861041

Page 3 of 3 Pages

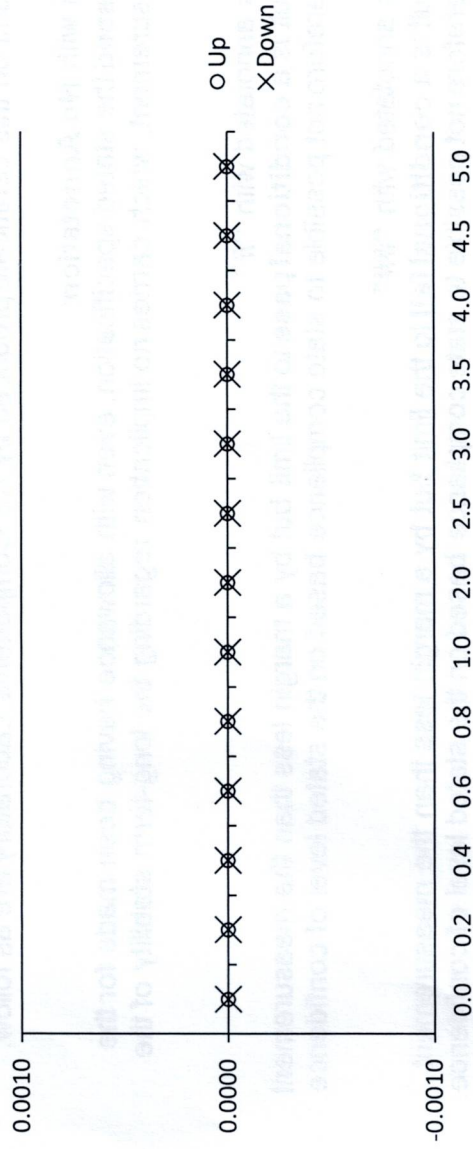

Reported values not annotated.

The instrument passed the stated specification, due allowance having been made for the uncertainty of measurement which carries no implication regarding the long term stability of the instrument.

END OF CALIBRATION

Appendix SCQAR533 Certificate Statements of conformity

RS Components is standardising how it reports conformity across all disciplines in line with requirements within **ISO/IEC: 17025:2017**. Where the laboratory reports a statement of conformity to a specification, guidance has been drawn on reporting structure and decision rules from ILAC document series **ILAC-G8:09/2019**. Unless otherwise instructed by you the Customer, acceptance limits applied are derived from the manufacturers specification or applicable standard (e.g. DIN, EEC, BS etc.) or where applicable: SCQAR532_RS Standard Limits for Calipers, available on request. The statements found on this certificate produced by RS Components Laboratory are as follow:

- 1) Reported values with **No Annotation**:
The instrument **passed** the stated specification, even with allowance having been made for the uncertainty of measurement, which carries no implication regarding the long-term stability of the instrument.
- 2) Reported values annotated with “#”
The measured result is a **conditional pass** to the limit but by a margin less than the measurement uncertainty, it is therefore not possible to state compliance based on the stated level of confidence.
- 3) Reported values annotated with “##”
The measured result is a **conditional fail** to the limit but by a margin less than the measurement uncertainty, it is therefore not possible to state compliance based on the stated level of confidence.
- 4) Reported values annotated with “###”
The measured result **failed** the stated specification, even with allowance having been made for the measurement uncertainty.

