

GAC



RS Calibration
Calibration and Repair Service
Serial No: 025400955
Cert No: 1872846
Cal Date: 11 Jul 2024
Recal Due:

DPN 175 Lammas Road, Corby, Northants, NN17 9RS

****Calibration Certificate****

Do Not Destroy

Calibration Certificate Attached: 1872846


OD ref: 1237504918

Eutechnics 4500 RTD thermometer

first

IMPORTANT INFORMATION

Simply detach the label in the top right hand corner of the new front sheet and apply to your instrument as required.

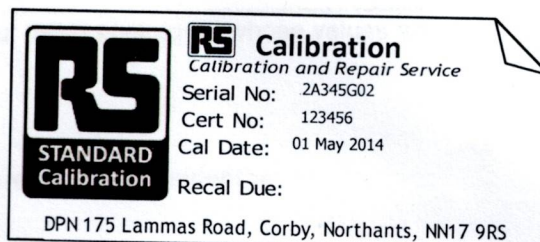

For Re-Calibration of your unit please email:

calibration.uk@rs-components.com

or call us on 01536 405545 to arrange free collection. Please quote serial number when returning.

RS Calibration

CERTIFICATE OF CALIBRATION

Issued by: RS Components Ltd

Date Issued: 11 Jul 2024

Certificate No. 1872846



RS Calibration

Calibration and Repair Service

DPN 175, Lammas Rd,
Weldon Industrial Est
Corby, Northants, NN17 9RS

Tel: 01536 405545

Fax: 01536 401590

Page 1 of 3 Pages

Gary Chadwick

Client	TOTAL LABORATORY SERVICES LTD BLANDFORD FORUM DORSET DT11 8ST
Instrument	Eutechnics 4500 RTD thermometer
Serial No.	025400955
Client Reference	N/A
Procedure ID.	X01_8241_(SYSC2_95%) Rev. P1
Probe Stock No.	N/A
Probe Description	Eutechnics SP 640, 110mm long metal sheathed NTC type probe. Serial No. 502723
Date of Calibration	11 Jul 2024

Equipment Used to Carry Out Calibration

Equipment ID.

Fluke 1586A Precision Temperature Scanner	Cal 1339
Fluke 1586-2588 DAQ-STAQ multiplexer	Cal 1340
HART 7340 high precision bath	Cal 1160
Platinum Resistance Probe	Cal 906, 1151

The measurements reported in this certificate were carried out using equipment whose values are traceable to national standards.

The management controls of the RS Calibration Laboratory are registered under the British Standard BS EN ISO 9001 : 2015 No. RS 00362.

Uncertainties

The reported expanded uncertainties are based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a level of confidence of approximately 95%.

This certificate reports recorded values for the instrument 'As Received'.

For certificate statements of conformity see Appendix SCQAR 533

The following calibration results relate only to the items defined above.

This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

CERTIFICATE OF CALIBRATION

Certificate No.

1872846



Calibration and Repair Service

Page 2 of 3 Pages

Environment

The ambient temperature and relative humidity throughout the calibration were $(21 \pm 3) ^\circ\text{C}$ and $(50 \pm 20) \%RH$ respectively.

Method

The instrument was calibrated by comparison with reference resistance probes in a stirred liquid medium bath set to 20°C , 30°C , 40°C , and 50°C .

The reference resistance probes were measured with resistance bridges to determine the true temperature of the test medium.

Prior to the calibration the instrument was allowed to stabilise in the laboratory for a period of not less than 30 minutes.

The immersion depth of the probe was not less than: 100 mm in stirred baths

The tested resolution of the instrument is as the displayed result.

Reference Measured Temperature	Instrument Indicated	Instrument Error	Measurement Uncertainties	Specification allowance
20.06 $^\circ\text{C}$	20.06 $^\circ\text{C}$	0.00 $^\circ\text{C}$ #	± 0.04 $^\circ\text{C}$	± 0.04 $^\circ\text{C}$
30.07 $^\circ\text{C}$	30.07 $^\circ\text{C}$	0.00 $^\circ\text{C}$ #	± 0.04 $^\circ\text{C}$	± 0.04 $^\circ\text{C}$
40.07 $^\circ\text{C}$	40.07 $^\circ\text{C}$	0.00 $^\circ\text{C}$ #	± 0.04 $^\circ\text{C}$	± 0.04 $^\circ\text{C}$
50.05 $^\circ\text{C}$	50.04 $^\circ\text{C}$	-0.01 $^\circ\text{C}$ #	± 0.04 $^\circ\text{C}$	± 0.04 $^\circ\text{C}$

CALIBRATED BY:- GAC

Reported values

The uncertainties quoted refer to the recorded values, which include any identified contribution of the instrument under test and not to the ability of the instrument to maintain its calibration.

Compliance to Specification

The specification used for the probe is found in :

The manufacturer's specification

is used in combination with the specification published by the manufacturer as found in the instrument's handbook and has been used to determine performance at the measured points.

CERTIFICATE OF CALIBRATION

Certificate No.
1872846

RS Calibration
Calibration and Repair Service

Page 3 of 3 Pages

Reported values not annotated

The instrument complies with the stated specification, due allowance having been made for the uncertainty of measurement which carries no implication regarding the long term stability of the instrument.

Reported values annotated with a

The measured result is a conditional pass to the specification limit by a margin less than the measurement uncertainty; it is therefore not possible to state compliance based on the stated level of confidence.

END OF CALIBRATION

IMPORTANT

INFORMATION

The equipment of this unit please email: rs@rs-calibration.com
rs-calibration.com
Please return the equipment to the address above.
When returning the equipment please include the serial number and the date of return.

Appendix SCQAR533 Certificate Statements of conformity

RS Components is standardising how it reports conformity across all disciplines in line with requirements within **ISO/IEC: 17025:2017**.

Where the laboratory reports a statement of conformity to a specification, guidance has been drawn on reporting structure and decision rules from ILAC document series **ILAC-G8:09/2019**.

Unless otherwise instructed by you the Customer, acceptance limits applied are derived from the manufacturers specification or applicable standard (e.g. DIN, EEC, BS etc.) or where applicable: SCQAR532_RS Standard Limits for Calipers, available on request.

The statements found on this certificate produced by RS Components Laboratory are as follow:

1) Reported values with **No Annotation**:

The instrument **passed** the stated specification, even with allowance having been made for the uncertainty of measurement, which carries no implication regarding the long-term stability of the instrument.

2) Reported values annotated with **"#"**

The measured result is a **conditional pass** to the limit but by a margin less than the measurement uncertainty, it is therefore not possible to state compliance based on the stated level of confidence.

3) Reported values annotated with **"##"**

The measured result is a **conditional fail** to the limit but by a margin less than the measurement uncertainty, it is therefore not possible to state compliance based on the stated level of confidence.

4) Reported values annotated with **"###"**

The measured result **failed** the stated specification, even with allowance having been made for the measurement uncertainty.

